


NANOCOLOR® Härte 20

Hardness 20 / Dureté 20 / Durezza 20











Test 0-43
REF 985043

Methode / Method / Méthode / Método

0431 1–20 °d
0432 0.2–3.6 mmol/L
0433 1.0–25.0 °e
0434 2.0–36.0 °f


540 / 570 nm

Min	20–80 %		Max
1	4.8	15.2	20 °d

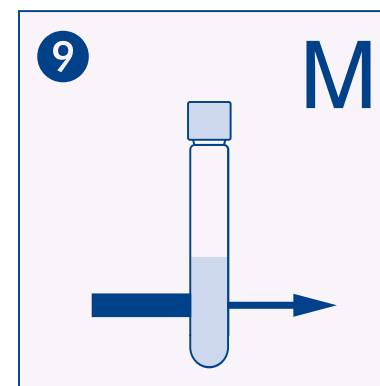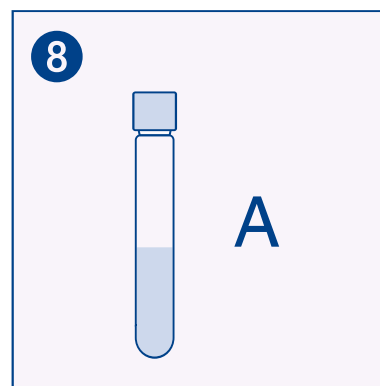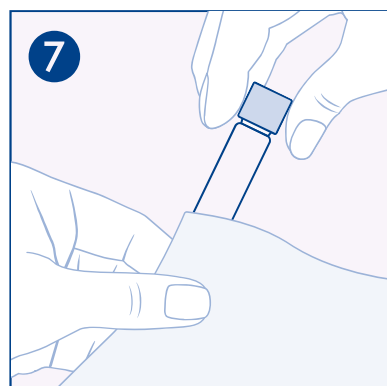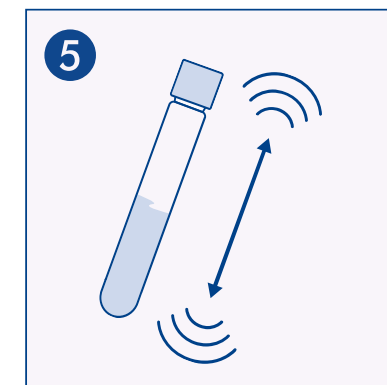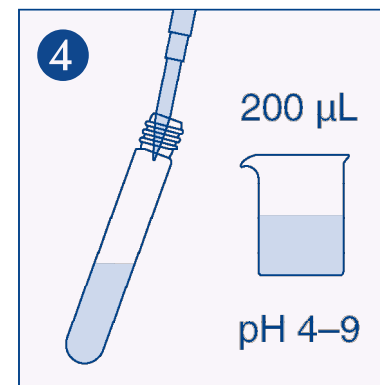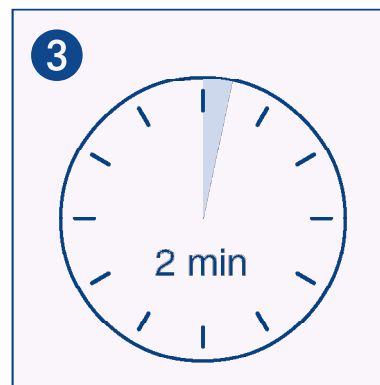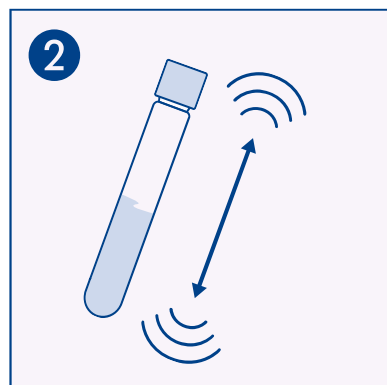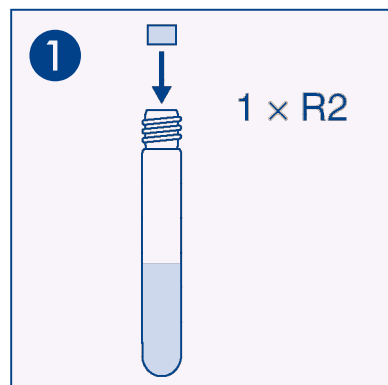

NANOCOLOR® Härte 20

Hardness 20 / Dureté 20 / Dureza 20



Test 0-43
REF 985043

Methode / Method / Méthode / Método

0435 10–100 mg/L Ca

0436 5–50 mg/L Mg

0437 20–350 mg/L CaCO₃

540 / 570 nm

Min	20–80 %		Max
10	28	82	100 mg/L Ca
5	14	45	50 mg/L Mg

