


MACHEREY-NAGEL

# User manual





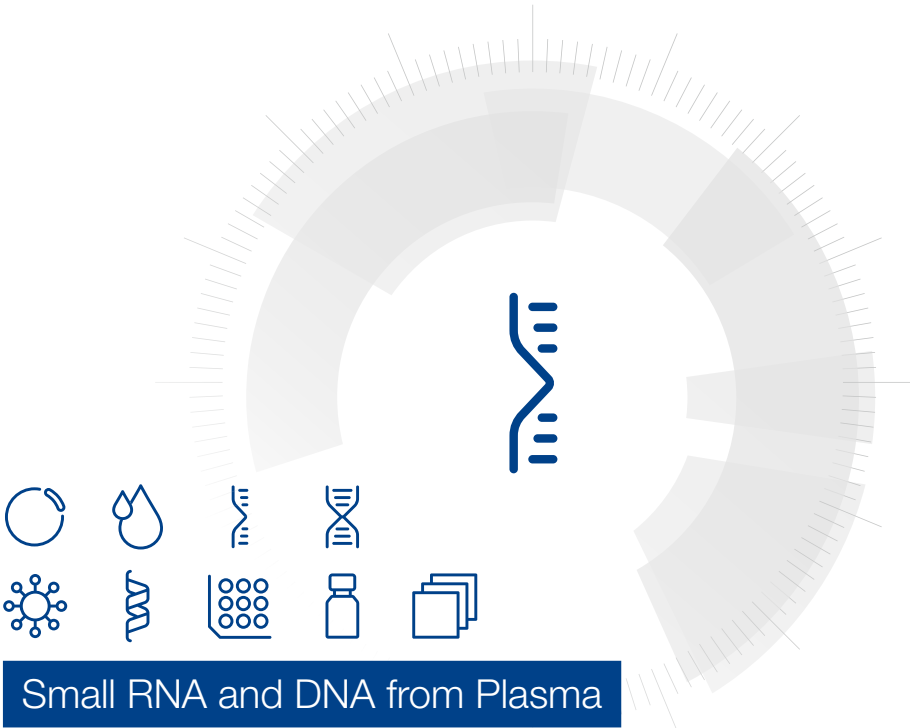











## Small RNA and DNA from Plasma

- NucleoSpin® miRNA Plasma

November 2023 / Rev. 08

# Isolation of miRNA from plasma

## Protocol at a glance (Rev.08)

		<b>NucleoSpin® miRNA Plasma</b>
<b>1 Prepare sample</b>		300 µL plasma or serum* 90 µL MLP Vortex 5 s RT, 3 min
<b>2 Precipitate protein</b>	 	30 µL MPP Vortex 5 s RT, 1 min 11,000 x g, 3 min
<b>3 Transfer supernatant</b>		Transfer clear supernatant to Collection Tube (2 mL, lid)
<b>4 Adjust binding conditions</b>	 	400 µL isopropanol Vortex 5 s
<b>5 Bind RNA and DNA</b>	 	Load sample on NucleoSpin® miRNA Column RT, 2 min 11,000 x g, 30 s
<b>6 Optional: Digest DNA</b>	 	<b>Optional:</b> <div style="display: flex; flex-direction: column; gap: 10px;"> <div> <b>1<sup>st</sup></b> 700 µL MW2            11,000 x g, 30 s         </div> <div> <b>2<sup>nd</sup></b> 250 µL MW2            11,000 x g, 2 min         </div> </div> 50 µL rDNase in Reaction Buffer for rDNase RT, 15 min
<b>7 Wash and dry</b>	 	<div style="display: flex; flex-direction: column; gap: 10px;"> <div> <b>1<sup>st</sup></b> 100 µL MW1            11,000 x g, 30 s         </div> <div> <b>2<sup>nd</sup></b> 700 µL MW2            11,000 x g, 30 s         </div> <div> <b>3<sup>rd</sup></b> 250 µL MW2            11,000 x g, 2 min         </div> </div>
<b>8 Elute RNA</b>	 	30 µL RNase-free H <sub>2</sub> O RT, 1 min 11,000 x g, 1 min

\* Larger sample volumes can be processed when buffer volumes of MLP, MPP, and isopropanol are increased proportionally. Multiple loading is necessary in step 5 (see section 2.3 for more information).

## Table of contents

1	Components	4
1.1	Kit contents	4
1.2	Reagents, consumables, and equipment to be supplied by user	5
1.3	About this user manual	5
2	Product description	6
2.1	The basic principle	6
2.2	Kit specifications	6
2.3	Amount of starting material	6
2.4	Proteinase K digest	8
2.5	Addition of carrier	8
2.6	Elution procedures	8
3	Storage conditions and preparation of working solutions	9
4	Safety instructions	10
4.1	Disposal	10
5	Protocol - small RNA and DNA purification from plasma or serum	11
6	Appendix	14
6.3	Product use restriction / warranty	16
6.1	Troubleshooting	14
6.2	Ordering information	15
6.3	Product use restriction / warranty	16

# 1 Components

## 1.1 Kit contents

<b>NucleoSpin® miRNA Plasma</b>			
<b>REF</b>	<b>10 preps 740981.10</b>	<b>50 preps 740981.50</b>	<b>250 preps 740981.250</b>
Lysis Buffer MLP	3 mL	13 mL	75 mL
Protein Precipitation Buffer MPP	5 mL	5 mL	25 mL
Reaction Buffer for rDNase	7 mL	7 mL	30 mL
rDNase, RNase-free (lyophilized)	1 vial (size C)	1 vial (size C)	5 vials (size C)
Wash Buffer MW1	10 mL	10 mL	35 mL
Wash Buffer MW2 (Concentrate)*	6 mL	25 mL	100 mL
RNase-free H <sub>2</sub> O	13 mL	13 mL	13 mL
NucleoSpin® miRNA Columns (green rings)	10	50	250
Collection Tubes (1.5 mL)	10	50	250
Collection Tubes (2 mL)	10	50	250
Collection Tubes (2 mL, lid)	10	50	250
User manual	1	1	1

\* For preparation of working solutions and storage conditions see section 3.

## 1.2 Reagents, consumables, and equipment to be supplied by user

### Reagents

- 96–100 % ethanol
- Isopropanol

### Consumables

- RNase-free disposable pipette tips

### Equipment

- Manual pipettors
- Vortexer
- Centrifuge for microcentrifuge tubes
- Personal protection equipment (lab coat, gloves, goggles)

## 1.3 About this user manual

It is strongly recommended that first-time users of the **NucleoSpin® miRNA Plasma** kit read the detailed protocol section of this user manual. Experienced users, however, may refer to the Protocol at a glance instead. The Protocol at a glance is designed to be used only as a supplemental tool for quick referencing while performing the purification procedure.

All technical literature is available on the internet at [www.mn-net.com](http://www.mn-net.com).

## 2 Product description

### 2.1 The basic principle

The **NucleoSpin® miRNA Plasma** kit offers the unique feature to isolate total RNA including small RNA and DNA from serum and plasma without the need to resort to the cumbersome phenol/chloroform extraction or a time consuming proteinase digest.

The sample material is denatured in Lysis Buffer MLP. The protein is then precipitated by Protein Precipitation Buffer MPP and pelleted by centrifugation.

After the removal of protein the binding conditions for nucleic acids are adjusted by adding isopropanol.

Total nucleic acids are bound to the NucleoSpin® miRNA Column. Optionally, DNA can be removed by an on-column rDNase digest. The remaining nucleic acids are washed and eluted with minimal amounts of RNase-free water.

### 2.2 Kit specifications

- The **NucleoSpin® miRNA Plasma** kit is designed for the isolation of RNA and DNA from cell free blood plasma or serum.
- **rDNase** is provided for an optional on-column digest to remove traces of genomic DNA.
- The eluted RNA and DNA are ready to use for all standard downstream applications, for example, qPCR, qRT-PCR, Northern Blot, chip hybridization.

**Table 1: Kit specifications at a glance**

Parameter	NucleoSpin® miRNA Plasma
Sample size	300 µL blood plasma or serum
Binding capacity	200 µg
Elution volume	20 – 50 µL
Preparation time	40 min/10 preps (without rDNase digest) 70 min/10 preps (with rDNase digest)
Use	For research use only


### 2.3 Amount of starting material

The standard procedure allows to process 300 µL of sample material with only one loading step onto the NucleoSpin® miRNA Column. This is usually enough to detect also low abundance miRNA in plasma or serum.

If larger sample volumes are to be used to increase the sensitivity even further, the volumes of Buffer MLP and Buffer MPP as well as the isopropanol have to be increased proportionally. Multiple loading steps per sample are necessary.

But, consider that doubling or tripling the starting volume will result in an only 1–1.5 cycles earlier signal in qRT-PCR, which is rather insignificant for detection sensitivity compared to the much larger differences that occur from sample to sample or between different miRNAs. Furthermore, if plasma quality is low, co-purified RT-PCR inhibitors might require diluting the eluate and thereby counteract the increased yields.

Figure 1 shows qRT-PCR results from eight different plasma samples analyzed for miR-16 (very high expression) and miR-1 (very low expression). They differ in average by about 14 cycles, which is a difference in expression by 3–4 orders of magnitude (1.000–10.000 fold)! Doubling the amount of sample material would just shift the mean values from 32.6 to 31.6 (miR-1) and from 18.3 to 17.3 (miR-16). This is much less than the variation from sample to sample and can thus be neglected.

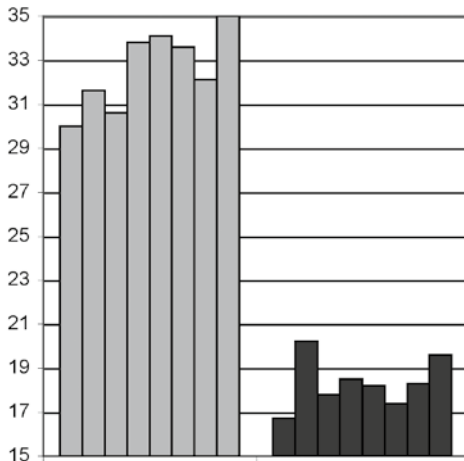

**Figure 1 qRT-PCR quantification of miR-1 and miR-16**

MiRNA from only 300  $\mu\text{L}$  of eight different blood plasma samples were purified and eluted in 30  $\mu\text{L}$  RNase-free water. 2  $\mu\text{L}$  of each eluate were used for a 10  $\mu\text{L}$  RT reaction (Applied Biosystems, TaqMan<sup>®</sup> MicroRNA RT Kit) with miRNA specific primers (Applied Biosystems, hsa-miR-1 MicroRNA Assay and hsa-miR-16 MicroRNA Assay). The RT reaction mix was diluted 1:10. Only 4  $\mu\text{L}$  of the resulting 100  $\mu\text{L}$  were used for the PCR reaction (Applied Biosystems TaqMan<sup>®</sup> Universal PCR Master Mix) in combination with the MicroRNA Assays for specific priming mentioned before.

### 2.3.1 Preparation of plasma from human EDTA blood

- 1 Centrifuge fresh blood sample for 10 min at 2,000  $\times g$ .
- 2 Remove the plasma without disturbing sedimented cells.
- 3 Freeze plasma at -20  $^{\circ}\text{C}$  for storage upon RNA isolation.
- 4 Thaw frozen plasma samples prior to RNA isolation and centrifuge for 3 min at  $\geq 11,000 \times g$  in order to remove residual cells, cell debris, and particulate matter. Use the supernatant for RNA isolation.

## 2.4 Proteinase K digest

A short protein digestion step might increase miRNA yield, especially for low quality, hemolyzed plasma. Add 10  $\mu\text{L}$  of Proteinase K (~ 30  $\mu\text{g}/\mu\text{L}$  in Buffer PB, see ordering information) to 300  $\mu\text{L}$  plasma, incubate for 10 min at 37 °C, and then proceed with addition of Buffer MLP according to the protocol.

## 2.5 Addition of carrier

To improve RNA/DNA binding to the NucleoSpin® miRNA Column, carrier can be added to the sample after the removal of precipitated protein. Slightly higher yields could be found with 2  $\mu\text{g}$  of glycogen or 5  $\mu\text{g}$  of LPA (linear polyacrylamide). However, negligible effects were observed for Poly-A which furthermore interferes with a photometric quantification of the purified nucleic acids.

## 2.6 Elution procedures

The elution buffer volume does not only influence total yield and concentration of RNA and DNA, but does also influence the ratio between very small and larger oligonucleotides:

### 20 $\mu\text{L}$

The silica membrane is not completely wetted. Only weakly binding very small oligonucleotides like miRNA are eluted efficiently. Larger RNA and DNA are more likely to remain bound to the column. The eluted miRNA is highly concentrated.

### 30 $\mu\text{L}$ (standard)

The standard elution buffer volume of 30  $\mu\text{L}$  is sufficient to wet the silica membrane completely. It results a high total yield of miRNA / RNA / DNA and simultaneously maximizes the concentration.

### 50 $\mu\text{L}$

Increasing the elution buffer volume will further increase the final yield but consequently will reduce the concentration. The gain in yield will usually not compensate for the loss in sensitivity of miRNA detection caused by the dilution of the eluate. Furthermore, larger RNA and DNA will be eluted more efficiently, which might, however, be interesting for the analysis of circulating DNA.



### 3 Storage conditions and preparation of working solutions

**Attention:**

*Buffers MLP and MW1 contain guanidinium thiocyanate. Wear gloves and goggles!*

Storage conditions:

- Store lyophilized RNase-free rDNase at +4 °C on arrival (stable for at least one year).
- All other kit components should be stored at 15–25 °C and are stable until: see package label. Storage at lower temperatures may cause precipitation of salts.

Before starting the first **NucleoSpin® miRNA Plasma** procedure prepare the following:

- **Wash Buffer MW2:** Add the indicated volumes of 96–100 % ethanol to the MW2 concentrate. The buffer can be stored at room temperature (15–25 °C) for at least one year.
- **RNase-free rDNase:** Add the indicated volume of Reaction Buffer for rDNase to the rDNase vial and incubate for 1 min at room temperature. Gently swirl the vial to completely dissolve the rDNase. Be careful not to mix rDNase vigorously as rDNase is sensitive to mechanical agitation. Dispense into aliquots and store at -20 °C. The frozen solution is stable for at least 6 months. Do not freeze/thaw the aliquots more than three times.

NucleoSpin® miRNA Plasma			
REF	10 preps 740981.10	50 preps 740981.50	250 preps 740981.250
Wash Buffer MW2 (Concentrate)	6 mL Add 24 mL ethanol	25 mL Add 100 mL ethanol	100 mL Add 400 mL ethanol
RNase-free rDNase (lyophilized)	1 vial (size C) Add 3 mL Reaction Buffer for rDNase	1 vial (size C) Add 3 mL Reaction Buffer for rDNase	5 vials (size C) Add 3 mL Reaction Buffer for rDNase to each vial

## 4 Safety instructions

When working with the **NucleoSpin® miRNA Plasma** kit wear suitable protective clothing (e.g., lab coat, disposable gloves, and protective goggles). For more information consult the appropriate Material Safety Data Sheets (MSDS available online at [www.mn-net.com/msds](http://www.mn-net.com/msds)).



Caution: Guanidinium thiocyanate in buffer MLP and buffer MW1 can form highly reactive compounds when combined with bleach! Thus, do not add bleach or acidic solutions directly to the sample preparation waste.

The waste generated with the **NucleoSpin® miRNA Plasma** kit has not been tested for residual infectious material. A contamination of the liquid waste with residual infectious material is highly unlikely due to strong denaturing lysis buffer treatment but it cannot be excluded completely. Therefore, liquid waste must be considered infectious and should be handled and discarded according local safety regulations.

### 4.1 Disposal

Dispose hazardous, infectious or biologically contaminated materials in a safe and acceptable manner and in accordance with all local and regulatory requirements.

## 5 Protocol - small RNA and DNA purification from plasma or serum

Before starting with the preparation check that isopropanol is available, that ethanol was added to Wash Buffer MW2, and that rDNase was reconstituted according to section 3.

### 1 Prepare sample


*Note:* See section 2.4 for optional Proteinase K digest.

Add **90  $\mu$ L Buffer MLP** to **300  $\mu$ L sample**.

Vortex for **5 s**.

Incubate for **3 min** at **room temperature**.

*Note:* To process 600  $\mu$ L or 900  $\mu$ L sample material, increase volumes for Buffer MLP, MPP, and isopropanol proportionally. Multiple loading steps will be necessary in step 5. See section 2.3 for more information.




### 2 Precipitate protein

Add **30  $\mu$ L Buffer MPP** and vortex for **5 s**.

Incubate for **1 min** at **room temperature**.

Centrifuge for **3 min** at **11,000 x g** to pellet the protein.



### 3 Transfer supernatant


Transfer the clear supernatant into a new Collection Tube (2 mL, lid).



### 4 Adjust binding conditions

*Note:* Addition of carrier, for example, 2  $\mu$ g of glycogen or 5  $\mu$ g of LPA (linear polyacrylamide), might slightly improve the miRNA yield but usually is not necessary. Poly-A has shown only negligible effects and furthermore might interfere with photometric miRNA quantification.

Add **400  $\mu$ L isopropanol** and vortex for **5 s**.



**5 Bind RNA and DNA**

Place a **NucleoSpin® miRNA Column** in a Collection Tube (2 mL) and load the sample onto the column.

Incubate for **2 min** at **room temperature**.

Centrifuge for **30 s** at **11,000 x g**.

Discard the flowthrough and place the column back into the collection tube.

If more than 300 µL plasma/serum was used, repeat this step until all sample is loaded onto the column.



**Load sample**

**RT**  
**2 min**



**11,000 x g**  
**30 s**

**Repeat step if necessary**

**6 Optional: DNA digest**

*Note: Co-purified DNA might interfere with qPCR quantification of miRNA. The following on-column digest degrades bound DNA including miRNA genes.*

However, if miRNA specific qPCR detection systems are used or cell free plasma DNA is needed intact for further analysis, skip the rDNase digest and proceed directly with step 7.

**1<sup>st</sup> wash**

Add **700 µL Buffer MW2** to the NucleoSpin® miRNA Column. Centrifuge for **30 s** at **11,000 x g**. Discard flowthrough and place the column back into the collection tube.



**+ 700 µL MW2**



**11,000 x g**  
**30 s**

**2<sup>nd</sup> wash**

Add **250 µL Buffer MW2** to the NucleoSpin® miRNA Column. Centrifuge for **2 min** at **11,000 x g**. It is not necessary to discard the flowthrough.



**+ 250 µL MW2**



**11,000 x g**  
**2 min**

**Digest DNA**

Add **50 µL rDNase** (dissolved in Reaction Buffer for rDNase according to section 3) directly onto the silica membrane of the NucleoSpin® miRNA Column.



**+ 50 µL rDNase**



**RT**  
**15 min**

Close the lid and incubate at **room temperature** for **15 min**.

**7 Wash and dry silica membrane****1<sup>st</sup> wash**



Add **100 µL Buffer MW1** to the NucleoSpin® miRNA Column. Centrifuge for **30 s** at **11,000 x g**.

Discard flowthrough and place the column back into the collection tube.

**2<sup>nd</sup> wash**

Add **700 µL Buffer MW2** to the NucleoSpin® miRNA Column. Centrifuge for 30 s at **11,000 x g**.

Discard flowthrough and place the column back into the collection tube.



**3<sup>rd</sup> wash**

Add **250 µL Buffer MW2** to the NucleoSpin® miRNA Column.

Centrifuge for **2 min** at **11,000 x g** to dry the membrane completely.

If the liquid in the collection tube has touched the NucleoSpin® miRNA Column after the 3<sup>rd</sup> wash, discard flowthrough and centrifuge again.

*Note: The same collection tube is used throughout the entire washing procedure to reduce plastic waste. If new collection tubes are to be used for each step, see ordering information.*

**8 Elute RNA and DNA**


Place the NucleoSpin® miRNA Column in a new Collection Tube (1.5 mL).

*Note: The elution buffer volume highly influences the final yield and concentration and, furthermore, influences elution efficiency of large oligonucleotides. See section 2.6 for more information about elution in 20, 30 or 50 µL.*

Add **30 µL RNase-free H<sub>2</sub>O** directly onto the silica membrane of the column.

Incubate for **1 min** at **room temperature**.

Close the lid and centrifuge for **1 min** at **11,000 x g**.



## 6 Appendix

### 6.1 Troubleshooting

Problem	Possible cause and suggestions
Poor or no RNA yield	<i>Reagents not applied or restored properly</i>
	<ul style="list-style-type: none"> <li>• Always dispense exactly the buffer volumes given in the protocols! The correct proportions of buffers MLP, MPP, and isopropanol are essential for optimal yield and purity.</li> <li>• Always follow closely the given instructions with regard to order and mode of mixing (shaking, vortexing etc).</li> <li>• Add the indicated volume of 96 – 100 % ethanol to Buffer MW2 Concentrate and mix thoroughly.</li> <li>• Store kit components at room temperature . Storage at lower temperatures may cause salt precipitation. Heat buffer with precipitated salt to 30 °C until salt is dissolved. Let the buffer cool down to room temperature before use.</li> <li>• Keep bottles tightly closed in order to prevent evaporation or contamination.</li> </ul>
	<i>RNase contamination</i>
	RNA is degraded
Suboptimal performance of RNA in downstream experiments	<p data-bbox="288 979 684 1002"><i>Inhibition by co-purified RT-PCR inhibitors</i></p> <ul style="list-style-type: none"> <li>• Heme, hemin, and other degradation products of red blood cells strongly inhibit reverse transcription and PCR. Too much plasma or bad plasma quality can result in contamination with these inhibitors. Use less plasma, dilute eluates, perform the optional Proteinase K digest (see section 2.4), or add BSA prior to RT or PCR reactions.</li> </ul>

<b>Problem</b>	<b>Possible cause and suggestions</b>
Suboptimal performance of RNA in downstream experiments (continued)	<i>Carry-over of ethanol or salt</i>
	<ul style="list-style-type: none"> <li>Do not let the flowthrough touch the column outlet after the second MW2 wash. Make sure to centrifuge at the corresponding speed for the respective time in order to remove ethanolic buffer MW2 completely.</li> <li>Check if buffer MW2 has been equilibrated to room temperature before use. Washing at lower temperatures lowers efficiency of salt removal.</li> </ul>
	<p><i>Store isolated RNA properly</i></p> <ul style="list-style-type: none"> <li>Eluted RNA should always be kept on ice for optimal stability since trace contaminations of omnipresent RNases (general lab ware, fingerprints, dust) will degrade the isolated RNA. For short term storage freeze at -20 °C, for long term storage freeze at -70 °C.</li> </ul>

## 6.2 Ordering information

<b>Product</b>	<b>REF</b>	<b>Pack of</b>
NucleoSpin® miRNA Plasma	740981.10/.50/.250	10/50/250 preps
Exosome Precipitation Solution (Serum/Plasma)	740398.12/.20/.60	12/20/60 mL
Exosome Precipitation Solution (Urine)	740399.12/.50/.250	12/50/250 mL
NucleoSpin® miRNA	740971.10/.50/.250	10/50/250 preps
rDNase Set (1 vial rDNase (size F), 7 mL Reaction Buffer for rDNase)	740963	1 set
Proteinase K	740506	100 mg
Collection Tubes (2 mL)	740600	1000

Visit [www.mn-net.com](http://www.mn-net.com) for more detailed product information.

### 6.3 Product use restriction/warranty

All MACHEREY-NAGEL products are designed for their intended use only. They are not intended to be used for any other purpose. The description of the intended use of the products can be found in the original MACHEREY-NAGEL product leaflets. Before using our products, please observe the instructions for use and the safety instructions from the respective Material Safety Data Sheet of the product.

This MACHEREY-NAGEL product is carrying documentation stating specifications and other technical information. MACHEREY-NAGEL warrants to meet the stated specifications. The provided warranty is limited to the data specifications and descriptions as given in the original MACHEREY-NAGEL literature. No other statements or representations, written or oral, by MACHEREY-NAGEL's employees, agents or representatives, except written statements signed by a duly authorized officer of MACHEREY-NAGEL are authorized. They should not be relied upon by the customer and are not a part of a contract of sale or of this warranty.

Liability for all possible damages that occur in any connection with our products is limited to the utmost minimum as stated in the general business terms and conditions of MACHEREY-NAGEL in their latest edition which can be taken from the company's website. MACHEREY-NAGEL does not assume any further warranty.

Products and their application are subject to change. Therefore, please contact our Technical Service Team for the latest information on MACHEREY-NAGEL products. You may also contact your local distributor for general scientific information. Descriptions in MACHEREY-NAGEL literature are provided for informational purposes only.

Last updated: 08/2022, Rev. 04

Please contact:

MACHEREY-NAGEL GmbH & Co. KG

Tel.: +49 24 21 969-333

support@mn-net.com

---


Trademarks/Disclaimer:

NucleoSpin® is a registered trademark of MACHEREY-NAGEL GmbH & Co. KG


TaqMan® is a registered trademark of Roche Molecular Systems, Inc.

All used names and denotations can be brands, trademarks, or registered labels of their respective owner – also if they are not special denotation. To mention products and brands is only a kind of information (i.e., it does not offend against trademarks and brands and can not be seen as a kind of recommendation or assessment). Regarding these products or services we can not grant any guarantees regarding selection, efficiency, or operation.



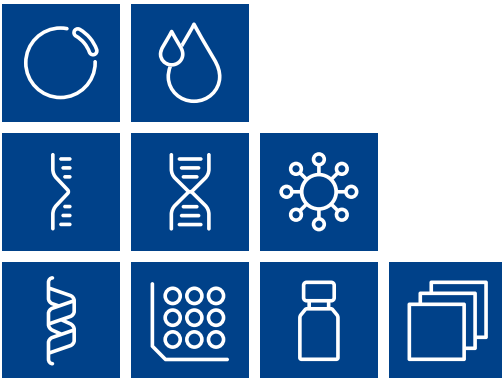

Plasmid DNA  
Clean up  
RNA  
DNA  
Viral RNA and DNA  
Protein  
High throughput  
Accessories  
Auxiliary tools

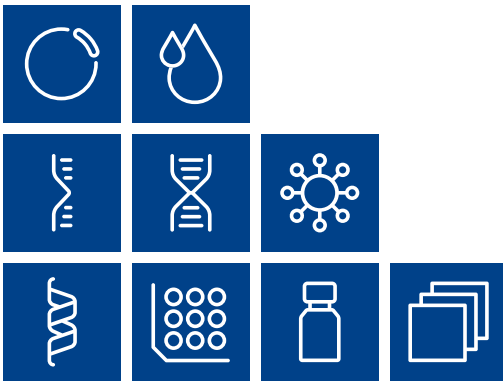

[www.mn-net.com](http://www.mn-net.com)

**MACHEREY-NAGEL**



A040554/1130.x



MACHEREY-NAGEL GmbH & Co. KG · Valenciener Str. 11 · 52355 Düren · Germany

DE +49 24 21 969-0 [info@mn-net.com](mailto:info@mn-net.com)

CH +41 62 388 55 00 [sales-ch@mn-net.com](mailto:sales-ch@mn-net.com)

FR +33 388 68 22 68 [sales-fr@mn-net.com](mailto:sales-fr@mn-net.com)

US +1 888 321 62 24 [sales-us@mn-net.com](mailto:sales-us@mn-net.com)