


MACHEREY-NAGEL

# User manual

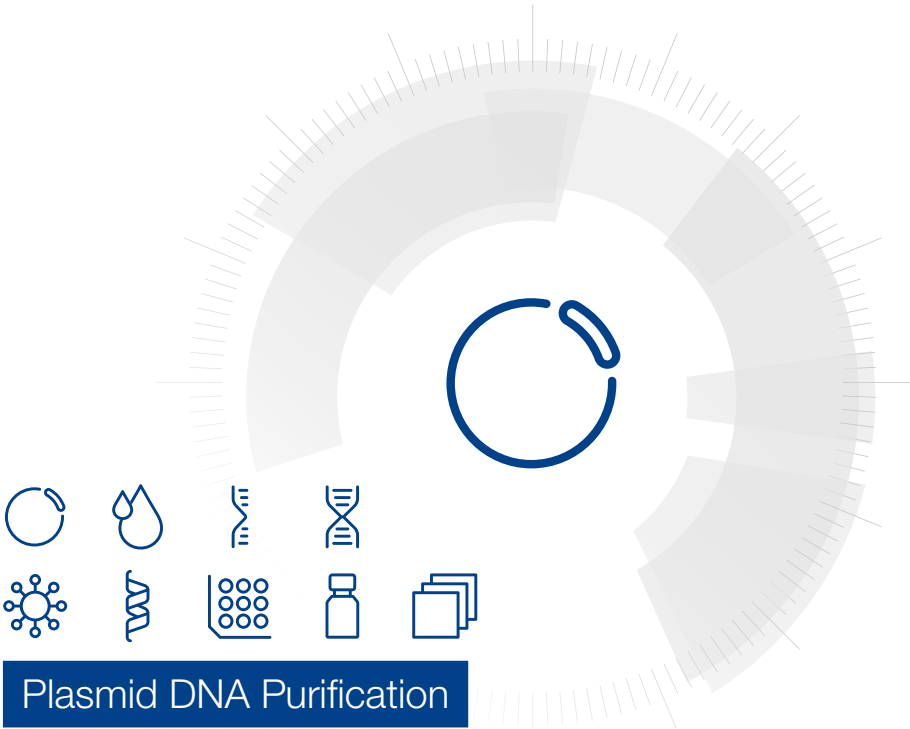

## Plasmid DNA Purification

■ NucleoMag® Plasmid

May 2024 / Rev. 01

## Contact MN

### Germany and international

MACHEREY-NAGEL GmbH & Co. KG  
Valenciener Str. 11 · 52355 Düren · Germany  
Tel.: +49 24 21 969-0  
Toll-free: 0800 26 16 000 (Germany only)  
E-mail: [info@mn-net.com](mailto:info@mn-net.com)

### Technical Support Bioanalysis

Tel.: +49 24 21 969-333  
E-mail: [support@mn-net.com](mailto:support@mn-net.com)

### USA

MACHEREY-NAGEL Inc.  
924 Marcon Blvd. · Suite 102 · Allentown PA, 18109 · USA  
Toll-free: 888 321 6224 (MACH)  
E-mail: [sales-us@mn-net.com](mailto:sales-us@mn-net.com)

### France

MACHEREY-NAGEL SAS  
1, rue Gutenberg – BP135 · 67720 Hoerdt Cedex · France  
Tel.: +33 388 68 22 68  
E-mail: [sales-fr@mn-net.com](mailto:sales-fr@mn-net.com)

MACHEREY-NAGEL SAS (Société par Actions Simplifiée) au capital de 186600 €  
Siret 379 859 531 00020 · RCS Strasbourg B379859531 · N° intracommunautaire FR04 379 859 531

### Switzerland

MACHEREY-NAGEL AG  
Hirsackerstr. 7 · 4702 Oensingen · Switzerland  
Tel.: +41 62 388 55 00  
E-mail: [sales-ch@mn-net.com](mailto:sales-ch@mn-net.com)

## Table of contents

1 Components	4
1.1 Kit contents	4
1.2 Reagents, consumables, and equipment to be supplied by user	4
1.3 About this user Manual	5
2 Product description	6
2.1 Basic principle	6
2.2 Kit specifications	7
2.3 Automated processing on robotic platforms	8
2.4 Growth of bacterial cultures	8
2.5 Lysate clearance	8
2.6 Handling of beads	9
2.7 Elution procedures	9
3 Storage conditions and preparation of working solutions	10
4 Safety instructions	11
4.1 Disposal	11
5 Protocol for isolation of plasmid DNA	12
5.1 General overview	12
5.2 Overview	12
6 Protocols for magnetic rod systems	15
6.1 General information	15
6.2 General setup for magnetic rod systems	15
6.3 Detailed protocols for IsoPure™ Mini and MagnetaPure32 Plus	16
6.3.1 Protocol for lysate clearance via centrifugation	16
6.3.2 Protocol for lysate clearance via magnetic beads	20
6.4 Detailed protocols for KingFisher™ Flex	23
6.4.1 Protocol for lysate clearance via centrifugation	23
6.4.2 Protocol for lysate clearance via magnetic beads	25
6.5 Support protocol for transfection-grade plasmid DNA isolation	28
6.5.1 Support protocol for IsoPure™ Mini and MagnetaPure32 Plus (TG)	28
6.5.2 Support protocol for KingFisher™ Flex (TG)	31
7 Appendix	34
7.1 Troubleshooting	34
7.2 Ordering information	37
7.3 Product use restriction / warranty	38

# 1 Components

## 1.1 Kit contents

NucleoMag® Plasmid		
REF	1 × 96 preps 744750.1	4 × 96 preps 744750.4
Resuspension Buffer A1	15 mL	75 mL
Lysis Buffer A2	15 mL	100 mL
Neutralization Buffer S3	25 mL	100 mL
Binding Buffer PAB	2 × 35 mL	300 mL
NucleoMag® M-Beads	2 × 1 mL	8 × 1 mL
Detoxification Buffer ERB	2 × 125 mL	2 × 400 mL
Wash Buffer AQ (Concentrate)*	2 × 25 mL	2 × 100 mL
Elution Buffer AE**	30 mL	60 mL
RNase A (lyophilized)*	12 mg	60 mg
Leaflet	1	1

## 1.2 Reagents, consumables, and equipment to be supplied by user

### Reagents

- 96 – 100 % ethanol (non-denatured)
- Lysate clarification via magnetic beads: NucleoMag® Clearing Beads (REF: 744751.1)
- Endotoxin-free water H<sub>2</sub>O-EF (REF 740798.1) or ddH<sub>2</sub>O

### Consumables

#### *Lysate clarification via centrifugation*

- 2 mL microcentrifuge tubes for sample lysis

\* For preparation of working solutions and storage conditions, see section 3.

\*\* Composition of Elution Buffer AE: 5mM Tris/HCl, pH 8.5

or

- 96 deep-well plate suitable for centrifugation (e.g. Square well Block REF: 740481)
- 96 deep-well plate suitable for the respective magnetic rod instrument
- Rod sleeves/Tip combs suitable for the respective magnetic rod instrument

*KingFisher™ Flex*

- 96-well Accessory Kit A for KingFisher™ (REF: 744950)

*IsoPure™ Mini/MagnetaPure32 Plus*

- 96-Deep-Well plates for magnetic rod systems (REF: 744955)
- 8-well Tip Combs for magnetic rod systems (REF: 744960)

### Equipment

- 8-channel pipette or dispenser pipette for setup of reagent plates

*Lysate clarification via centrifugation*

- Centrifuge for microcentrifuge tubes

or

- Centrifuge with swing-bucket rotor capable of at least  $2,000 \times g$  (optimal  $4,000 \times g$ ) in combination with the compatible rotor and rotor buckets for 96-well deep-well plates

## 1.3 About this user Manual

It is strongly recommended that first time users of the **NucleoMag® Plasmid** kit read the detailed protocol sections of this user manual. Experienced users, however, may refer to the Protocol at a glance instead. The Protocol at a glance is designed to be used as a tool for quick referencing while performing the purification procedure.

All technical literature is available at [www.mn-net.com](http://www.mn-net.com).

Please contact Technical Service regarding information about changes of the current user manual compared to previous revisions.

## 2 Product description

### 2.1 Basic principle

The **NucleoMag® Plasmid** procedure utilizes a modified alkaline lysis protocol in combination with the reversible adsorption of nucleic acids to paramagnetic beads under appropriate buffer conditions. Pelleted bacteria are resuspended in Buffer A1. Plasmid DNA is liberated from the cells by Lysis Buffer A2 followed by a subsequent neutralization and precipitation of the lysate using Buffer S3. The crude lysate can be cleared either by centrifugation or using NucleoMag® Clearing Beads, specialized paramagnetic beads for lysate clearing. For binding of nucleic acids to the paramagnetic beads, Binding Buffer PAB and the NucleoMag® M-Beads are added to the cleared lysate. After magnetic separation, endotoxins and proteins are removed by the patented Detoxification Buffer ERB. Further contaminations such as salts or residual ethanol are removed with Wash Buffer AQ and air drying. Pure plasmid DNA is eluted with low-salt elution buffer or water and is ready for any common downstream application including transfection (research use only). The **NucleoMag® Plasmid** kit has been designed for the use on automated magnetic rod-systems.

## 2.2 Kit specifications

**NucleoMag® Plasmid** kit is designed for the rapid automated small-scale purification of transfection-grade plasmid DNA from *E. coli* using magnetic-rod systems. The kit allows for easy automation on common magnetic rod instruments such as KingFisher™ systems, MagnetaPure32 Plus, IsoPure Mini or others.

**Table 1: Kit specifications at a glance**

Parameter	NucleoMag® Plasmid
Technology	Magnetic bead technology
Format	Magnetic beads
Sample material	≤ 5 mL <i>E. coli</i> culture
Typical yield	1 – 50 µg, depending on copy number, plasmid size, culture media, culture condition and bacterial host strain
Typical purity	$A_{260}/A_{280} \geq 1.8$ $A_{260}/A_{230} \geq 2.0$
Typical Endotoxin level	Lysate clearance via centrifugation – 3 wash steps: ≤ 50 EU/µg  Lysate clearance via centrifugation – 4 wash steps: ≤ 10 EU/µg  Lysate clearance via magnetic beads: ≤ 50 EU/µg
Vector size	< 25 kbp
Elution volume	50 – 200 µL
Preparation time	Depending on instrument type, script and configuration
Processing	Automated
Use	For research use only

## 2.3 Automated processing on robotic platforms

The NucleoMag® Plasmid kit has been designed for the use on magnetic rod-based instruments, such as the KingFisher™ systems, Auto-Pure, MagnetaPure32 Plus or IsoPure™ instruments.

The use of the NucleoSpin® 8/96 Plasmid (Transfection-grade) kits is recommended in combination with liquid handling platforms equipped with vacuum manifolds or a positive pressure unit, due to the lower tip consumption, full automation and processing time.

For the availability of scripts and general considerations about adaptations to a certain instrument, please contact MN.

Visit MN online at [www.mn-net.com](http://www.mn-net.com) or contact your local MACHEREY-NAGEL distributor for technical support regarding hardware, software, setup, instructions and selection of the protocol.

## 2.4 Growth of bacterial cultures

Plasmid yield and quality highly depend on the bacterial culture which is influenced by many factors. Besides culture medium, selective antibiotic, bacterial host strain and type of plasmid, the oxygen availability is of crucial importance for bacterial growth. Anaerobic metabolism of nutrients will result in suboptimal energy uptake and accumulation of organic acids as metabolic end products which inhibit further cell growth.

When incubating bacterial cultures in small volumes with limited surface (as in a 96-deep-well plates or culture plates (see ordering information section 7.2), take care to shake the plates vigorously (200–400 rpm) to maintain a proper aeration of the culture. To avoid cross contamination due to spillage during incubation, cover the 96-deep-well plate with a gas-permeable foil (supplied with culture plate). Do not exceed a total culture volume of 1.5 mL (recommended volume approx. 1 mL) when working with the culture plates. If an increased total culture volume is desired, it is possible to grow bacteria in several culture plates with identical layout or in 24 deep-well plates. Either way take care not to exceed the total resuspension volume of 150 µL per sample. The total volume of 150 µL per sample may either be split into the corresponding number of plates and pooled after resuspension or the total amount may directly be dispensed into a first plate and completely transferred to succeeding plates after resuspension.

The **NucleoMag® Plasmid** kit is optimized for the purification of plasmid DNA from volumes between 1 – 1.5 mL of bacterial cultures but can be used with up to 5 mL with an OD<sub>600</sub> of 4 or up to 3 mL of a culture with an OD<sub>600</sub> of 8. Cultures with a higher OD<sub>600</sub> can be used by reducing the sample volume to 0.5 mL. Using significantly more bacteria without adapting the protocol will overload the lysis capacity, complicate bead resuspension and result in reduced yield and purity.

## 2.5 Lysate clearance

The NucleoMag® Plasmid kit offers two options for lysate clearance. The most common process of lysate clearance displays the centrifugation of neutralized lysate and the subsequent transfer of the cleared lysate to a fresh reaction vessel or plate.



Alternatively, lysate clearance can be performed by using NucleoMag® Clearing Beads during the neutralization and clarification step. Cellular debris and other contaminants are aggregated by the NucleoMag® Clearing Beads and removed from the supernatant via magnetic separation.

Both options possess advantages and disadvantages in respect to their versatility, hands-on-time, and purity of plasmid DNA.

Method	Culture volume	OD <sub>600</sub> (Maximum)	Purity	Hands-on-time
Centrifugation	0.5–5 mL	4–8	+++	+
Magnetic beads	0.5–1.5 mL	3	+	++

## 2.6 Handling of beads

### Distribution of beads

A homogeneous distribution of the magnetic beads (NucleoMag® Clearing Beads, NucleoMag® M-Beads) into the individual wells of the separation plate is essential for a high well-to-well consistency. Therefore, before dispensing the beads, make sure that the beads are completely resuspended. Vortex the storage tubes vigorously and check if the beads are completely resuspended.

### Magnetic separation time

Attraction of the magnetic beads to the magnetic rods depends on the magnetic strength of the rods, the geometry of the rod sleeve and the processing plate. The individual times for complete attraction of the beads to the magnetic rods should be checked and adjusted on each system. A slower magnetic separation and a longer separation time is recommended to reduce bead carry over.

## 2.7 Elution procedures

Purified plasmid DNA can be eluted directly with the supplied Elution Buffer AE (5 mM Tris/HCl, pH 8.5). Elution can be carried out in a volume of  $\geq 50 \mu\text{L}$ . It is essential to cover the NucleoMag® M-Beads completely with elution buffer during the elution step. The volume of dispensed elution buffer depends on the magnetic rod system (e.g., the geometry of the rod sleeve and plate used). For efficient elution, the magnetic bead pellet should be resuspended completely in the elution buffer. For some separators, higher elution volumes might be necessary to cover the whole pellet and reduce the dead volume of the rod sleeve. A second magnetic separation or a slower magnetic separation is recommended to reduce bead carry over.

### 3 Storage conditions and preparation of working solutions

**Attention:** Buffer PAB contains guanidinium thiocyanate! **Wear gloves and goggles!**

CAUTION: Buffer PAB contains guanidinium thiocyanate, which can form highly reactive compounds when combined with bleach (sodium hypochloride). DO NOT add bleach or acidic solutions directly to the sample preparation waste.

- Store NucleoMag® M-Beads upon arrival at 2–8 °C.
- All other components can be stored at 15–25 °C and are stable until: see package label.
- Always keep buffer bottles tightly closed.
- Sodium dodecyl sulfate (SDS) in **Buffer A2** may precipitate if stored at temperatures below 20 °C. Precipitated SDS might form a firm layer at the bottom of the bottle, which is difficult to see from the side or above. Invert the bottle carefully several times (avoid extensive foaming) and check the bottom and solution for white flocculates. If a precipitate is observed in Buffer A2, incubate bottle at 30–40 °C for several minutes and mix well.
- Buffer ERB may form crystals. The crystals must be redissolved by heating to 50–60 °C whilst shaking. The bottle should be always closed during the heat incubation.  
Before starting the extraction process, the ERB buffer must be cooled down to room-temperature.

Before starting the **NucleoMag® Plasmid** protocol, prepare the following:

- **Wash Buffer AQ:** Add the indicated volume of ethanol (96–100 %) to Buffer AQ Concentrate before use. Mark the label of the bottle to indicate that ethanol was added. Store Wash Buffer AQ at 15–25 °C for up to one year.
- **RNase A:** Add 1 mL of Buffer A1 to the RNase A vial and vortex. Transfer the resulting solution into the buffer A1 bottle and mix thoroughly. Indicate the date of RNase A addition. Store Buffer A1 containing RNase A at 2–8 °C for up to 6 months.

NucleoMag® Plasmid		
REF	1 × 96 preps 744750.1	4 × 96 preps 744750.4
Wash Buffer AQ (Concentrate)	2 × 25 mL Add 100 mL ethanol to each bottle	2 × 100 mL Add 400 mL ethanol to each bottle

## 4 Safety instructions

When working with the NucleoMag® Plasmid kit wear suitable protective clothing (e.g., lab coat, disposable gloves, and protective goggles). For more information consult the appropriate Material Safety Data Sheets (MSDS available online at [www.mn-net.com/msds](http://www.mn-net.com/msds)).



Caution: Guanidinium thiocyanate in buffer PAB can form highly reactive compounds when combined with bleach! Thus, do not add bleach or acidic solutions directly to the sample preparation waste.

The waste generated with the NucleoMag® Plasmid kit has not been tested for residual infectious material. A contamination of the liquid waste with residual infectious material is highly unlikely due to strong denaturing lysis buffer treatment but it cannot be excluded completely. Therefore, liquid waste must be considered infectious and should be handled and discarded according to local safety regulations.

### 4.1 Disposal

Dispose hazardous, infectious or biologically contaminated materials in a safe and acceptable manner and in accordance with all local and regulatory requirements.

## 5 Protocol for isolation of plasmid DNA

### 5.1 General overview

The NucleoMag® Plasmid kit is specially designed for the use on magnetic rod systems, such as the KingFisher™, Auto-Pure, MagnetaPure32 Plus, IsoPure Mini or other magnetic rod-based instruments.

The use of the NucleoSpin® 8/96 Plasmid (Transfection-grade) kits is recommended in combination with liquid handling platforms equipped with vacuum manifolds or a positive pressure unit, due to the lower tip consumption, degree of automation and lower processing time.

For manual preparations the use of the NucleoSpin® Plasmid (Transfection-grade) kit is recommended.

Please contact our application support team (automation-bio@mn-net.com) for method files or more detailed information on specific automation platforms.

### 5.2 Overview

This overview highlights the different protocol options for magnetic rod devices.

Typical EU-level	Lysate clarification via Centrifugation		Lysate clarification via NucleoMag® Clearing Beads
	≤ 50 EU/μg	≤ 10 EU/μg	≤ 50 EU/μg
<b>1 Cultivate and harvest bacterial cells</b>	0.5 mL–5 mL LB or up to 2.5 mL 2 x YT or TB  5 min, 11,000 × g (2 mL tubes)  5 min, 4,000 × g (96 deep-well plate)		0.5 mL–1.5 mL LB or 2 x YT or TB  5 min, 11,000 × g (2 mL tubes)  5 min, 4,000 × g (96 deep-well plate)
<b>2 Resuspend bacterial cells</b>	150 μL A1  Mix or shake		90 μL A1  Resuspension on instrument
<b>3 Lyse bacterial cells</b>	150 μL A2  RT, 2 – 5 min  Mix, invert 5 times or shake gently		120 μL A2  Lysis on instrument
<b>4 Neutralize</b>	210 μL S3  Mix, invert 10 times or shake gently		120 μL S3  Neutralization on instrument

<b>5 Clarify lysate</b>	Centrifugation	Magnetic Beads
	10 min, 11,000 × <i>g</i> (2 mL tubes)	35 µL NucleoMag® Clearing Beads, magnetic separation
	10 min, 4,000 × <i>g</i> (96 deep-well plate)	
<b>6 Transfer cleared lysate</b>	Transfer up to 450 µL of cleared lysate	Removal of cellular debris via NucleoMag® Clearing Beads
<b>7 Bind DNA to NucleoMag® M-Beads</b>	20 µL NucleoMag® M-Beads and 530 µL PAB	20 µL NucleoMag® M-Beads and 390 µL PAB
	<i>Mix and resuspend for at least 5 min</i>	<i>Mix and resuspend for at least 5 min</i>
	Remove supernatant after 1 min separation	Remove supernatant after 1 min separation
<b>8 Wash with ERB</b>	900 µL ERB	900 µL ERB
	<i>Mix and resuspend for 2–5 min</i>	<i>Mix and resuspend for 2–5 min</i>
	Remove supernatant after 1 min separation	Remove supernatant after 1 min separation
<b>9 2<sup>nd</sup> Wash with ERB</b>	– 900 µL ERB	900 µL ERB
	<i>Mix and resuspend for 2–5 min</i>	<i>Mix and resuspend for 2–5 min</i>
	– Remove supernatant after 1 min separation	Remove supernatant after 1 min separation
<b>10 1<sup>st</sup> Wash with AQ</b>	900 µL AQ	900 µL AQ
	<i>Mix and resuspend for 2–5 min</i>	<i>Mix and resuspend for 2–5 min</i>
	Remove supernatant after 1 min separation	Remove supernatant after 1 min separation
<b>11 2<sup>nd</sup> Wash with AQ</b>	900 µL AQ	900 µL AQ
	<i>Mix and resuspend for 2–5 min</i>	<i>Mix and resuspend for 2–5 min</i>
	Remove supernatant after 1 min separation	Remove supernatant after 1 min separation

<b>12</b> Dry the beads	15 min, room temperature	15 min, room temperature
-------------------------	--------------------------	--------------------------

<b>13 Elute</b> Plasmid DNA	100 µL AE	100 µL AE
	<i>Mix and resuspend for at least 5 min</i>	<i>Mix and resuspend for at least 5 min</i>
	Transfer the eluate after 2–5 min separation to a new reaction vessel	Transfer the eluate after 2–5 min separation to a new reaction vessel

## 6 Protocols for magnetic rod systems

### 6.1 General information

The NucleoMag® Plasmid kit is specially designed for the use on magnetic rod systems, such as the KingFisher™, Auto-Pure, MagnetaPure32 Plus, IsoPure Mini or other magnetic rod-based instruments.

The use of the NucleoSpin® 8/96 Plasmid (Transfection-grade) kits is recommended in combination with liquid handling platforms equipped with vacuum manifolds or a positive pressure unit, due to the lower tip consumption, degree of automation and lower processing time.

Please contact our application support team (automation-bio@mn-net.com) for method files or more detailed information on specific automation platforms.

### 6.2 General setup for magnetic rod systems

- This overview serves as a guideline for the general setup of plates, columns, or reaction vessels of the respective instrument for the NucleoMag® Plasmid kit. Depending on the instrument, lysis of sample material can either be performed on the instrument or externally. Positions can represent different formats that are defined by the protocol and instrument (e.g., complete plates (96-well format devices, e.g. KingFisher™ Flex), single rows (12-well format), single columns (8-well format, e.g. MagnetaPure32 Plus, IsoPure™ Mini) or individual wells; cartridge-based systems). Depending on the degree of automation, the setup can differ substantially.

Position	Step	Buffer	Volume
1	Lysis/Binding	Cleared lysate, PAB, M-Beads	1000 µL
2	1 <sup>st</sup> Wash	ERB	900 µL
	<i>Optional Wash</i>	<i>ERB</i>	<i>900 µL</i>
3	2 <sup>nd</sup> Wash	AQ	900 µL
4	3 <sup>rd</sup> Wash	AQ	900 µL
5	Elution	AE	100 µL

## 6.3 Detailed protocols for IsoPure™ Mini and MagnetaPure32 Plus

*Note:* The required method files for processing the NucleoMag® Plasmid kit on the IsoPure™ Mini or MagnetaPure32 Plus instrument are available at the [qr.mn-net.com/qr/\(241\)744750.1](http://qr.mn-net.com/qr/(241)744750.1) or can be requested at [support@mn-net.com](mailto:support@mn-net.com).



Two protocol options utilizing different options for lysate clearance (centrifugation or magnetic beads) are available for processing the **NucleoMag® Plasmid** kit on the IsoPure™ Mini or MagnetaPure32 Plus instruments (see section 2.5). Please note, that reagent volumes, plate setup and script differ substantially between these two options. Please make sure to choose the correct script.

### 6.3.1 Protocol for lysate clearance via centrifugation

For hardware requirements and additional consumables, refer to sections 1.2.

#### Before starting the preparation:

- Check if RNase A was added to buffer A1 according to section 3.
- Check buffers A2 and ERB for precipitates according to section 3.
- Check if Wash buffer AQ was prepared according to section 3.
- Check if 96-Deep-Well plates for magnetic rod systems (REF: 744955) and 8-well Tip Combs for magnetic rod systems (REF: 744960) are available.
- Check if the correct script is installed on your instrument.
  - IsoPure™ Mini: NMPlasmid
  - MagnetaPure32 Plus: NMPlasmid

---

#### 1 Cultivate and harvest bacterial cells

Centrifuge the bacterial cultures for **5 min** at **11,000 x g** (2 mL tubes) or 5 min at 4,000 x g (96 deep-well plate)

Centrifugation at higher *g*-forces might produce tight pellets which are more difficult to resuspend.

Discard supernatant. Remove residual medium by tapping tube or plate upside down on a clear paper sheet or soft tissue.

*Note:* It is important to remove as much residual media as possible in order to ensure low endotoxin concentrations.

---



## 2 Resuspend bacterial cells

Add **150 µL Buffer A1 with RNase A**. Resuspend the cell pellet completely by vortexing, shaking or mixing by pipetting up and down. Resuspend bacterial cells completely.

*Note: No clumps should be visible.*

---

## 3 Lyse bacterial cells

Add **150 µL Buffer A2**. Incubate at **room temperature** for a maximum of **5 min** with moderate shaking (300 rpm).

*Note: Do not vortex to avoid shearing of genomic DNA. Do not allow the lysis reaction to proceed for more than 5 min.*

---

## 4 Neutralize

Add **210 µL Buffer S3**. Mix by pipetting up and down, inverting several times or shaking.

*Note: Do not vortex to avoid shearing of genomic DNA.*

---

## 5 Clarify lysate


Centrifuge for **10 min at 11,000 × g** (2 mL tubes) / **10 min at 4,000 × g** (96 deep-well plate) at room temperature. Proceed with step 6 in the meantime.

*Note: Centrifugation speeds depend on the used reaction vessel. E.g. a 96-deep-well plate: < 5,000 × g; 2 mL tubes: 11,000 × g. Please check the compatibility of the used centrifuge beforehand.*

---

## 6 Prepare reagent plate(s)

Prepare the reagent plate(s) for IsoPure™ or MagnetaPure32 Plus instruments according to the following loading scheme:

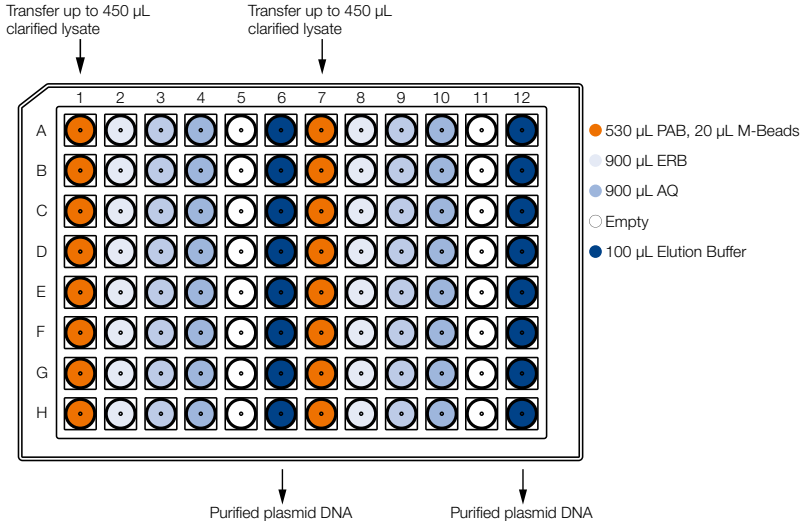

Column 1 and 7: Fill **530  $\mu$ L Buffer PAB** and **20  $\mu$ L M-Beads** to each well

Column 2 and 8: Fill **900  $\mu$ L Detoxification Buffer ERB** to each well

Column 3 and 9: Fill **900  $\mu$ L Wash Buffer AQ** to each well

Column 4 and 10: Fill **900  $\mu$ L Wash Buffer AQ** to each well

Column 6 and 12: Fill **100  $\mu$ L Elution Buffer AE** to each well

*Note: Do not moisten the upper rim of the 96 deep-well plate.*

## 7 Transfer cleared lysate

Transfer up to **450  $\mu$ L** of **cleared lysate** to column 1 and 7 of the prepared reagent plate for IsoPure™ or MagnetaPure32 Plus instruments.

*Note: Avoid transferring white flocculants into the reagent plate.*

---

**8 Select the respective protocol and start the run**

IsoPure™ Mini : NMPlasmid

MagnetaPure32 Plus : NMPlasmid

Load the plate(s) on the instrument.

Insert tip combs on the mounting grooves.

Start the run

---

**9 Transfer eluate**

The instrument stops after the final elution step. Remove and discard tip combs. Unload the plate(s) from the instrument and transfer the eluate for further processing into a suitable plate or vessel.

---

## 6.3.2 Protocol for lysate clearance via magnetic beads

### Before starting the preparation:

- Check if RNase A was added to buffer A1 according to section 3.
- Check buffers A2 and ERB for precipitates according to section 3.
- Check if Wash buffer AQ was prepared according to section 3.
- Check if 96-Deep-Well plates for magnetic rod systems (REF: 744955) and 8-well Tip Combs for magnetic rod systems (REF: 744960) are available.
- Check if NucleoMag® Clearing Beads (REF: 744751.1) are available.
- Check if the correct script is installed on your instrument.
  - IsoPure™ Mini: NMPlasmidCB

*Note:* The script includes two manual interventions for the addition of Neutralization buffer S3 and Binding Buffer PAB.

---

### 1 Cultivate and harvest bacterial cells

Centrifuge 0.5 – 1.5 mL bacterial cultures for **5 min** at **11,000 x g (2 mL tubes)** or **5 min at 4,000 x g** (96 deep-well plate).

Prepare the reagent plate according to step 2 in the meantime.


Centrifugation at higher *g*-forces might produce tight pellets which are more difficult to resuspend.

Discard supernatant. Remove residual medium by tapping tube or plate upside down on a clear paper sheet or soft tissue.

*Note:* It is important to remove as much residual media as possible in order to ensure low endotoxin concentrations.

---

## 2 Prepare reagent plate(s)

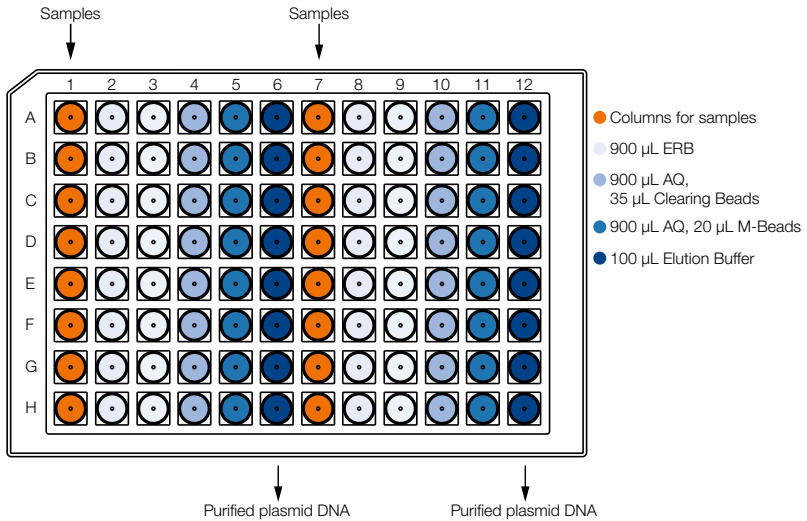

Prepare the reagent plate(s) for IsoPure™ instruments according to the following loading scheme:

Column 2 and 8: Fill **900 µL Detoxification Buffer ERB** to each well

Column 3 and 9: Fill **900 µL Detoxification Buffer ERB** to each well

Column 4 and 10: Fill **900 µL Wash Buffer AQ** and **35 µL NucleoMag® Clearing Beads** to each well

Column 5 and 11: Fill **900 µL Wash Buffer AQ** and **20 µL NucleoMag® M-Beads** to each well

Column 6 and 12: Fill **100 µL Elution Buffer AE** to each well

*Note: Do not moisten the upper rim of the 96 deep-well plate.*

## 3 Resuspend bacterial cells

Add **90 µL Buffer A1 with RNase A**. Resuspend the cell pellet completely by vortexing, shaking or mixing by pipetting up and down. Resuspend bacterial cells completely.

*Note: No clumps should be visible.*

## 4 Transfer samples to reagent plate

Transfer the resuspended bacterial cells into the respective well of column 1 or column 7.

*Note: Do not moisten the rim of the reagent plate.*

## 5 Lyse bacterial cells

Select the protocol from the instrument menu:

IsoPure™ Mini: NMPlasmidCB

Add **120 µL Buffer A2** to the resuspended bacterial cells in column 1 and 7. Immediately place the plate onto the instrument, insert tip combs on the mounting grooves and start the run.

*Note: Do not allow the lysis reaction to proceed for more than 2 min before placing the plates onto the instrument*

*Note: Please equip all tip combs to protect the magnetic rods in used and unused wells.*

---

## 6 Neutralize and lysate clearance

Dispense **120 µL Buffer S3** into the wells of column 1 and 7 when prompted. Continue the run.

*Note: Do not allow the lysis reaction to proceed for more than 5 min in total.*

---

## 7 Add Binding Buffer PAB

Dispense **390 µL Buffer PAB** into the wells of column 1 and 7 when prompted. Continue the run.

---

## 8 Transfer eluate

The instrument stops after the final elution step. Remove and discard tip combs. Unload the plate(s) from the instrument and transfer the eluate for further processing into a suitable plate or vessel.

---

## 6.4 Detailed protocols for KingFisher™ Flex

*Note:* The required method files for processing the **NucleoMag® Plasmid** kit on the KingFisher™ Flex instrument are available at the [qr.mn-net.com/qr/\(241\)744750.1](http://qr.mn-net.com/qr/(241)744750.1) or can be requested at [support@mn-net.com](mailto:support@mn-net.com)



Two protocol options utilizing different options for lysate clearance (centrifugation or magnetic beads) are available for processing the **NucleoMag® Plasmid** kit on the KingFisher™ Flex instruments (see section 2.5). Please note, that reagent volumes, plate setup and script differ substantially between these two options. Please make sure to choose the correct script.

### 6.4.1 Protocol for lysate clearance via centrifugation

#### Before starting the preparation:

- Check if RNase A was added to buffer A1 according to section 3.
- Check buffers A2 and ERB for precipitates according to section 3.
- Check if Wash buffer AQ was prepared according to section 3.
- Check if 96-well Accessory Kit A for KingFisher™ is available (REF: 744950)
- Check if the correct script is installed on your instrument.
- KingFisher™ Flex: NucleoMag\_Plasmid\_Flex

---

#### 1 Cultivate and harvest bacterial cells

Centrifuge the bacterial cultures for **5 min** at **4,000 x g** (96 deep-well plate).

Centrifugation at higher *g*-forces might produce tight pellets, which are more difficult to resuspend.

Discard supernatant. Remove residual medium by tapping tube or plate upside down on a clear paper sheet or soft tissue.

*Note:* It is important to remove as much residual media as possible in order to ensure low endotoxin concentrations.

---

#### 2 Resuspend bacterial cells

Add **150 µL Buffer A1 with RNase A**. Resuspend the cell pellet completely by vortexing, shaking or mixing by pipetting up and down. Resuspend bacterial cells completely.

*Note:* No clumps should be visible.

---

### 3 Lyse bacterial cells

Add **150 µL Buffer A2**. Incubate at **room temperature** for a maximum of **5 min** with moderate shaking (300 rpm).

*Note: Do not vortex to avoid shearing of genomic DNA. Do not allow the lysis reaction to proceed for more than 5 min.*

---

### 4 Neutralize

Add **210 µL Buffer S3**. Mix by pipetting up and down, inverting several times or shaking.

*Note: Do not vortex to avoid shearing of genomic DNA.*

---

### 5 Clarify lysate

Centrifuge for **10 min** at **4,000 × g** (96 deep-well plate) at room temperature. Proceed with step 6 in the meantime.

*Note: Centrifugation speeds depend on the used reaction vessel. E.g. a 96-deep-well plate < 5,000 × g. Please check the compatibility of the used centrifuge beforehand.*

---

### 6 Prepare reagent plate(s)

Prepare the reagent plate(s) for KingFisher™ Flex instruments according to the following loading scheme:

Plate 1: Fill **530 µL Buffer PAB** and **20 µL M-Beads** to each well of a deep-well plate for KingFisher™

Plate 2: Fill **900 µL Detoxification Buffer ERB** to each well of a deep-well plate for KingFisher™

Plate 3: Fill **900 µL Wash Buffer AQ** to each well of a deep-well plate for KingFisher™

Plate 4: Fill **900 µL Wash Buffer AQ** to each well of a deep-well plate for KingFisher™

Plate 5: Fill **100 µL Elution Buffer AE** to each well of an elution plate for KingFisher™

*Note: Do not moisten the upper rim of the 96 deep-well plate.*

---

### 7 Transfer cleared lysate

Transfer up to **450 µL** of cleared lysate to plate 1 of the prepared reagent plate for KingFisher™ Flex instruments.

*Note: Avoid transferring white flocculants into the reagent plate.*

---



## 8 Select the respective protocol and start the run

KingFisher™ Flex: NucleoMag\_Plasmid\_Flex

Load the plates as indicated on the KingFisher™ Flex instrument display.

Start the run.

---

## 9 Transfer eluate

The instrument stops after the final elution step. Remove and discard tip combs. Unload the plate(s) from the instrument and transfer the eluate for further processing into a suitable plate or vessel.

### 6.4.2 Protocol for lysate clearance via magnetic beads

#### Before starting the preparation:

- Check if RNase A was added to buffer A1 according to section 3.
- Check buffers A2 and ERB for precipitates according to section 3.
- Check if Wash buffer AQ was prepared according to section 3.
- Check if 96 Deep-well plates for magnetic rod systems (REF 744955) and Deep-well Tip Combs for KingFisher (REF 744956) are available.
- Check if NucleoMag® Clearing Beads (REF: 744751.1) are available.
- Check if the correct script is installed on your instrument.
- KingFisher™ Flex: NucleoMag\_Plasmid\_CB\_Flex

*Note:* The script includes two manual interventions for the addition of Neutralization buffer S3 and Binding Buffer PAB.

---

#### 1 Cultivate and harvest bacterial cells

Centrifuge 0.5 – 1.5 mL bacterial cultures for **5 min** at **4,000 x g (96 deep-well plate)**.

Prepare the reagent plates according to step 2 in the meantime.

Centrifugation at higher *g*-forces might produce tight pellets, which are more difficult to resuspend.

Discard supernatant. Remove residual medium by tapping tube or plate upside down on a clear paper sheet or soft tissue.

*Note:* It is important to remove as much residual media as possible in order to ensure low endotoxin concentrations.

---

## 2 Prepare reagent plates

Prepare the reagent plates for the KingFisher™ Flex instrument according to the following loading scheme:

Plate 2: Fill **900 µL Endotoxin-free water H<sub>2</sub>O-EF** to each well of a deep-well plate for KingFisher™.

Plate 3: Fill **900 µL Detoxification Buffer ERB** to each well of a deep-well plate for KingFisher™.

Plate 4: Fill **900 µL Detoxification Buffer ERB** to each well of a deep-well plate for KingFisher™.

Plate 5: Fill **900 µL Wash Buffer AQ** and **35 µL NucleoMag® Clearing Beads** to each well of a deep-well plate for KingFisher™.

Plate 6: Fill **900 µL Wash Buffer AQ** and **20 µL NucleoMag® M-Beads** to each well of a deep-well plate for KingFisher™.

Plate 7: Fill **100 µL Elution Buffer AE** to each well of an elution plate for KingFisher™.

*Note: Do not moisten the upper rim of the 96 deep-well plate.*

---

## 3 Resuspend bacterial cells

Add **90 µL Buffer A1 with RNase A**. Resuspend the cell pellet completely by vortexing, shaking or mixing by pipetting up and down. Resuspend bacterial cells completely.

*Note: No clumps should be visible.*

---

## 4 Transfer samples to reagent plate

Transfer the resuspended bacterial cells into the respective well of an empty deep-well plate for KingFisher™ (plate 1).

*Note: Do not moisten the rim of the reagent plate.*

---

## 5 Lyse bacterial cells

Select the protocol from the instrument menu:

KingFisher™ Flex: NucleoMag\_Plasmid\_CB\_Flex

Add **120 µL Buffer A2** to the resuspended bacterial cells in plate 1 using an 8-channel pipette or multi-dispensing pipette. Immediately place the plate onto the instrument, insert tip combs on the mounting grooves and start the run.

*Note: Do not allow the lysis reaction to proceed for more than 2 min before placing the plates onto the instrument*

---

---

**6 Neutralize and lysate clearance**

Dispense **120 µL Buffer S3** into the wells of **plate 1** when prompted. Continue the run.

*Note: Do not allow the lysis reaction to proceed for more than 5 min in total.*

---

**7 Add Binding Buffer PAB**

Dispense **390 µL Buffer PAB** into the wells of **plate 1** when prompted. Continue the run.

---

**8 Transfer eluate**

The instrument stops after the final elution step. Remove and discard tip combs. Unload the plates from the instrument and transfer the eluate for further processing into a suitable plate or vessel.

---

## 6.5 Support protocol for transfection-grade plasmid DNA isolation

The following support protocol utilizing only centrifugation for lysate clearance was designed to achieve plasmid DNA purifications with a typical endotoxin level  $\leq 10$  EU/  $\mu\text{g}$  Plasmid DNA. If endotoxin levels  $\leq 50$  EU/ $\mu\text{g}$  are sufficient, it is recommended to follow the standard procedure.

### 6.5.1 Support protocol for IsoPure™ Mini and MagnetaPure32 Plus (TG)

For hardware requirements and additional consumables, refer to sections 1.2.

#### Before starting the preparation:

- Check if RNase A was added to buffer A1 according to section 3.
- Check buffers A2 and ERB for precipitates according to section 3.
- Check if Wash buffer AQ was prepared according to section 3.
- Check if 96-Deep-Well plates for magnetic rod systems (REF: 744955) and 8-well Tip Combs for magnetic rod systems (REF: 744960) are available.
- Check if the correct script is installed on your instrument.

IsoPure™ Mini: NMPlasmidTG

MagnetaPure32 Plus: NMPlasmidTG

---

#### 1 Cultivate and harvest bacterial cells

*Centrifuge the bacterial cultures for 5 min at 11,000 × g (2 mL tubes) or 5 min at 4,000 × g (96 deep-well plate)*

*Centrifugation at higher g-forces might produce tight pellets which are more difficult to resuspend.*

*Discard supernatant. Remove residual medium by tapping tube or plate upside down on a clear paper sheet or soft tissue.*

*Note: It is important to remove as much residual media as possible to ensure low endotoxin concentrations. Repeat the centrifugation step to ensure the complete removal of residual media.*

---

#### 2 Resuspend bacterial cells

Add **150  $\mu\text{L}$  Buffer A1 with RNase A**. Resuspend the cell pellet completely by vortexing, shaking or mixing by pipetting up and down. Resuspend bacterial cells completely.

*Note: No clumps should be visible.*

---

### 3 Lyse bacterial cells

Add **150 µL Buffer A2**. Incubate at **room temperature** for a maximum of **5 min** with moderate shaking (300 rpm).

*Note: Do not vortex to avoid shearing of genomic DNA. Do not allow the lysis reaction to proceed for more than 5 min.*

---

### 4 Neutralize

Add 210 µL Buffer S3. Mix by pipetting up and down, inverting several times or shaking.

*Note: Do not vortex to avoid shearing of genomic DNA.*

---

### 5 Clarify lysate


Centrifuge for **10 min at 11,000 × g** (2 mL tubes) / **10 min at 4,000 × g** (96 deep-well plate) at room temperature. Proceed with step 6 in the meantime.

*Note: Centrifugation speeds depend on the used reaction vessel. E.g. a 96-deep-well plate: < 5,000 × g; 2 mL tubes: 11,000 × g. Please check the compatibility of the used centrifuge beforehand.*

---

## 6 Prepare reagent plate(s)

Prepare the reagent plate(s) for IsoPure™ or MagnetaPure32 Plus instruments according to the following loading scheme:

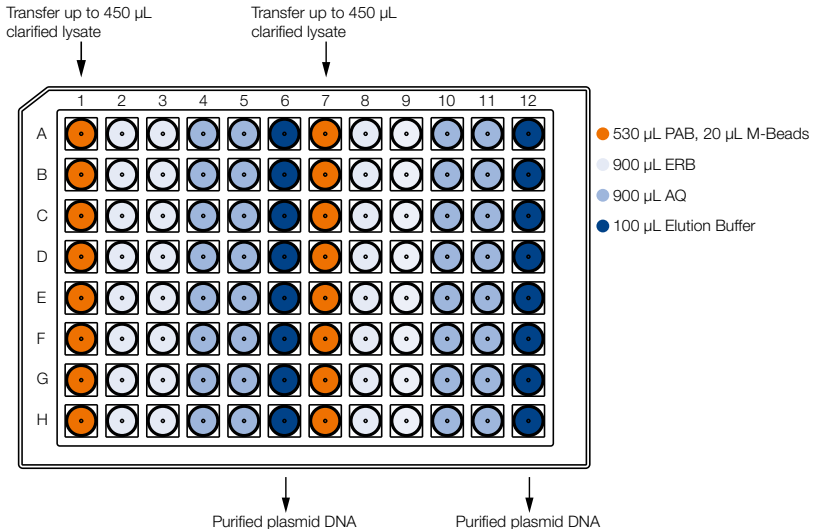

Column 1 and 7: Fill **530 µL Buffer PAB** and **20 µL M-Beads** to each well

Column 2 and 8: Fill **900 µL Detoxification Buffer ERB** to each well

Column 3 and 9: Fill **900 µL Detoxification Buffer ERB** to each well

Column 4 and 10: Fill **900 µL Wash Buffer AQ** to each well

Column 5 and 11: Fill **900 µL Wash Buffer AQ** to each well

Column 6 and 12: Fill **100 µL Elution Buffer AE** to each well

*Note: Do not moisten the upper rim of the 96 deep-well plate.*

## 7 Transfer cleared lysate

Transfer up to **450 µL** of **cleared lysate** to column 1 and 7 of the prepared reagent plate for IsoPure™ or MagnetaPure32 Plus instruments.

*Note: Avoid transferring white flocculants into the reagent plate.*

---

**8 Select the respective protocol and start the run**

IsoPure™ Mini : NMPlasmidTG

MagnetaPure32 Plus : NMPlasmidTG

Load the plate(s) on the instrument.

Insert tip combs on the mounting grooves.

Start the run

---

**9 Transfer eluate**

The instrument stops after the final elution step. Remove and discard tip combs. Unload the plate(s) from the instrument and transfer the eluate for further processing into a suitable plate or vessel.

---

## 6.5.2 Support protocol for KingFisher™ Flex (TG)

**Before starting the preparation:**

- Check if RNase A was added to buffer A1 according to section 3.
- Check buffers A2 and ERB for precipitates according to section 3.
- Check if Wash buffer AQ was prepared according to section 3.
- Check if 96-well Accessory Kit A for KingFisher™ is available (REF: 744950)
- Check if the correct script is installed on your instrument.

KingFisher™ Flex: NucleoMag\_Plasmid\_TG\_Flex

---

**1 Cultivate and harvest bacterial cells**

Centrifuge the bacterial cultures for **5 min** at **4,000 × g** (96 deep-well plate)

Centrifugation at higher *g*-forces might produce tight pellets which are more difficult to resuspend.

Discard supernatant. Remove residual medium by tapping tube or plate upside down on a clear paper sheet or soft tissue.

*Note: It is important to remove as much residual media as possible to ensure low endotoxin concentrations. Repeat the centrifugation step to ensure the complete removal of residual media.*

---

**2 Resuspend bacterial cells**

Add **150 µL Buffer A1 with RNase A**. Resuspend the cell pellet completely by vortexing, shaking or mixing by pipetting up and down. Resuspend bacterial cells completely.

*Note: No clumps should be visible.*

---

**3 Lyse bacterial cells**

Add **150 µL Buffer A2**. Incubate at **room temperature** for a maximum of **5 min** with moderate shaking (300 rpm).

*Note: Do not vortex to avoid shearing of genomic DNA. Do not allow the lysis reaction to proceed for more than 5 min.*

---

**4 Neutralize**

Add **210 µL Buffer S3**. Mix by pipetting up and down, inverting several times or shaking.

*Note: Do not vortex to avoid shearing of genomic DNA.*

---

**5 Clarify lysate**

Centrifuge for **10 min** at **11,000 × g** (2 mL tubes) / **10 min** at **4,000 × g** (96 deep-well plate) at room temperature. Proceed with step 6 in the meantime.

*Note: Centrifugation speeds depend on the used reaction vessel. E.g. a 96-deep-well plate: < 5,000 × g; 2 mL tubes: 11,000 × g. Please check the compatibility of the used centrifuge beforehand.*

---

**6 Prepare reagent plate(s)**

Prepare the reagent plate(s) for KingFisher™ Flex instruments according to the following loading scheme:

Plate 1: Fill **530 µL Buffer PAB** and **20 µL M-Beads** to each well of a deep-well plate for KingFisher™

Plate 2: Fill **900 µL Detoxification Buffer ERB** to each well of a deep-well plate for KingFisher™

Plate 3: Fill **900 µL Detoxification Buffer ERB** to each well of a deep-well plate for KingFisher™

Plate 4: Fill **900 µL Wash Buffer AQ** to each well of a deep-well plate for KingFisher™

Plate 5: Fill **900 µL Wash Buffer AQ** to each well of a deep-well plate for KingFisher™

Plate 6: Fill **100 µL Elution Buffer AE** to each well of an elution plate for KingFisher™

*Note: Do not moisten the upper rim of the 96 deep-well plate*

---

**7 Transfer cleared lysate**

Transfer up to 450 µL of cleared lysate to plate 1 of the prepared reagent plate for KingFisher™ Flex instruments.

*Note: Avoid transferring white flocculants into the reagent plate.*

---



---

**8 Select the respective protocol and start the run**

KingFisher™ Flex: NucleoMag\_Plasmid\_TG\_Flex

Load the plates as indicated on the KingFisher™ Flex instrument display.

Start the run

---

**9 Transfer eluate**

The instrument stops after the final elution step. Remove and discard tip combs. Unload the plate(s) from the instrument and transfer the eluate for further processing into a suitable plate or vessel.

---

## 7 Appendix

### 7.1 Troubleshooting

Problem	Possible cause and suggestions
	<i>Cell pellet not properly resuspended</i> <ul style="list-style-type: none"><li>It is essential that the cell pellet is completely resuspended prior to lysis. No cell clumps should be visible before addition of Buffer A2. Use the centrifugation speed and times given in the manual to avoid tight pellets.</li></ul>
	<i>SDS in Buffer A2 precipitated</i>
Incomplete lysis of bacterial cells	<ul style="list-style-type: none"><li>SDS in Buffer A2 may precipitate upon storage. If this happens a white precipitate is visible at the bottom of the bottle. Incubate Buffer A2 at 30–40 °C for several minutes and mix well before use.</li></ul>
	<i>Too many bacterial cells used</i> <ul style="list-style-type: none"><li>Usage of LB as the growth medium is recommended. When using rich media like 2 x YT or TB, cultures may reach very high cell densities. Reduce culture volume.</li></ul>

---

**Problem**

**Possible cause and suggestions**

---

	<p><i>Incomplete lysis of bacterial cells</i></p> <ul style="list-style-type: none"> <li>• See “Possible cause and suggestions” above</li> </ul> <p><i>No plasmid contained in bacteria</i></p> <ul style="list-style-type: none"> <li>• Cells carrying the plasmid of interest may become overgrown by non-transformed cells due to insufficient amounts of selective antibiotics.</li> <li>• Do not incubate cultures for more than 16 h as this may result in many dead and starving cells with degraded DNA.</li> </ul> <p><i>Use of low-copy plasmid</i></p> <ul style="list-style-type: none"> <li>• Getting acceptable plasmid yields for transfection requires high-copy plasmids in a miniprep scale or a switch to large scale kits (NucleoBond® Xtra Midi / Maxi).</li> <li>• <i>Suboptimal elution conditions</i></li> <li>• Elution efficiency will decrease with larger constructs. When working with large constructs, the elution buffer volume should be increased or the elution process should be prolonged.</li> </ul> <p><i>Suboptimal protocol conditions</i></p> <ul style="list-style-type: none"> <li>• Make sure to use verified scripts on the magnetic rod systems. Contact our support if script support is needed.</li> </ul> <p><i>Buffer AQ not prepared correctly</i></p> <ul style="list-style-type: none"> <li>• Add the indicated amount of 96–100 % ethanol to each bottle of Buffer AQ. Keep bottles closed tightly to prevent evaporation.</li> </ul>
<p>Genomic DNA contamination</p>	<p><i>Excessive mixing steps</i></p> <ul style="list-style-type: none"> <li>• Cell lysate was vortexed or mixed too vigorously after addition of Buffer A2 or Buffer S3. Genomic DNA was sheared and thus liberated.</li> <li>• Reduce number of mixing cycles, reduce shaker speed after addition of Lysis Buffer A2 and Neutralization Buffer S3. Excessive mixing can cause shearing of chromosomal DNA, leading to a copurification during the preparation of plasmid DNA.</li> </ul> <p><i>Lysis was too long</i></p> <ul style="list-style-type: none"> <li>• Lysis was too long and must not exceed 5 min.</li> </ul>

---

<b>Problem</b>	<b>Possible cause and suggestions</b>
RNA contamination	<p><i>RNA was not degraded completely</i></p> <ul style="list-style-type: none"> <li>• Ensure that RNase A was added to Buffer A1 and mixed well before use.</li> </ul>
Endotoxin levels are too high	<p><i>Carry over of residual cultivation media</i></p> <ul style="list-style-type: none"> <li>• Precisely remove the residual cultivation media after harvesting the cells. Perform a second centrifugation step and remove residual media.</li> </ul> <p>Suboptimal cultivation conditions</p> <ul style="list-style-type: none"> <li>• Optimize cultivation conditions in order the lower the amount of dead cells.</li> </ul>
Suboptimal performance in downstream applications	<p><i>Carry-over of ethanol from wash buffers</i></p> <ul style="list-style-type: none"> <li>• Be sure to remove all of the ethanolic wash solution, as residual ethanol interferes with downstream applications.</li> </ul> <p><i>RNA contamination</i></p> <ul style="list-style-type: none"> <li>• RNA might influence the photometric measurements resulting in an overestimation of plasmid DNA. Make sure RNase A is added to Buffer A1.</li> </ul>

## 7.2 Ordering information

Product	REF	Pack of
NucleoMag® Plasmid	744750.1	96 preps
	744750.4	384 preps
NucleoMag® Clearing Beads	744751.1	2 × 1.75 mL (96 preps)
Buffer A1 (without RNase A)	740911.1	1 L
Buffer A2 without LyseControl	740912.1	1 L
Buffer A2 with LyseControl	740328.100	100 mL
Buffer S3	740518.1	500 mL
Buffer AQ (Concentrate) (for 125 mL Buffer AQ)	740995	25 mL
H <sub>2</sub> O-EF	740798.1	1 L
RNase A (lyophilized)	740505	100 mg
	740505.50	50 mg
96-well Accessory Kit A for KingFisher™	744950	1 set
96 Deep-well plates for magnetic rod systems	744955	25
8-well Tip Combs for magnetic rod system	744960	50
Deep-well Tip Combs for KingFisher™	744956	4
Culture Plate (with Gas-permeable Foil)	740488	4 sets
	740488.24	24 sets
Gas-permeable Foil	740675	50
Self adhering Foil	740676	50

Visit [www.mn-net.com](http://www.mn-net.com) for more detailed product information.

## 7.3 Product use restriction / warranty

All MACHEREY-NAGEL products are designed for their intended use only. They are not intended to be used for any other purpose. The description of the intended use of the products can be found in the original MACHEREY-NAGEL product leaflets. Before using our products, please observe the instructions for use and the safety instructions from the respective Material Safety Data Sheet of the product.

This MACHEREY-NAGEL product is carrying documentation stating specifications and other technical information. MACHEREY-NAGEL warrants to meet the stated specifications. The provided warranty is limited to the data specifications and descriptions as given in the original MACHEREY-NAGEL literature. No other statements or representations, written or oral, by MACHEREY-NAGEL's employees, agents or representatives, except written statements signed by a duly authorized officer of MACHEREY-NAGEL are authorized. They should not be relied upon by the customer and are not a part of a contract of sale or of this warranty.

Liability for all possible damages that occur in any connection with our products is limited to the utmost minimum as stated in the general business terms and conditions of MACHEREY-NAGEL in their latest edition which can be taken from the company's website. MACHEREY-NAGEL does not assume any further warranty.

Products and their application are subject to change. Therefore, please contact our Technical Service Team for the latest information on MACHEREY-NAGEL products. You may also contact your local distributor for general scientific information. Descriptions in MACHEREY-NAGEL literature are provided for informational purposes only.

Last updated: 08/2022, Rev. 04

Please contact:  
MACHEREY-NAGEL GmbH & Co. KG  
Tel.: + 49 24 21 969-333  
support@mn-net.com

---

### Trademarks:


KingFisher is a registered trademark of Thermo Fisher Scientific

IsoPure is a registered trademark of Accuris Instruments


NucleoMag<sup>®</sup> is a registered trademark of MACHEREY NAGEL GmbH & Co. KG

NucleoSpin<sup>®</sup> is a registered trademark of MACHEREY NAGEL GmbH & Co. KG

All used names and denotations can be brands, trademarks, or registered labels of their respective owner – also if they are not special denotation. To mention products and brands is only a kind of information (i.e., it does not offend against trademarks and brands and can not be seen as a kind of recommendation or assessment). Regarding these products or services we can not grant any guarantees regarding selection, efficiency, or operation.

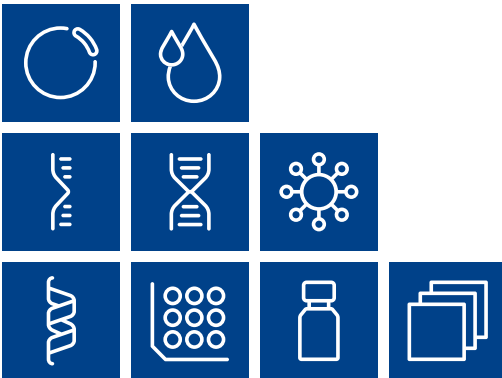

Plasmid DNA  
Clean up  
RNA  
DNA  
Viral RNA and DNA  
Protein  
High throughput  
Accessories  
Auxiliary tools

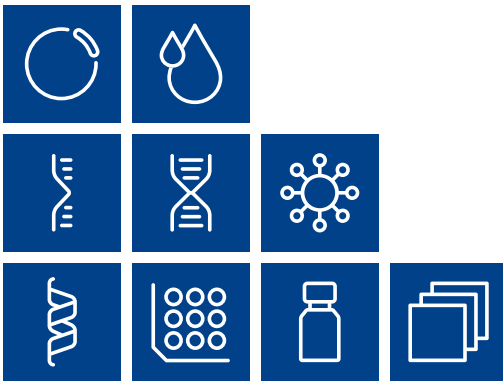

[www.mn-net.com](http://www.mn-net.com)

**MACHEREY-NAGEL**



MACHEREY-NAGEL GmbH & Co. KG · Valenciener Str. 11 · 52355 Düren · Germany

DE +49 24 21 969-0 [info@mn-net.com](mailto:info@mn-net.com)

CH +41 62 388 55 00 [sales-ch@mn-net.com](mailto:sales-ch@mn-net.com)

FR +33 388 68 22 68 [sales-fr@mn-net.com](mailto:sales-fr@mn-net.com)

US +1 888 321 62 24 [sales-us@mn-net.com](mailto:sales-us@mn-net.com)